

JUNCTION BOXES

AISI 304 STAINLESS STEEL




TÍN THÀNH TIẾN

LAUMAS®

www.laumas.com



- AISI 304 STAINLESS STEEL JUNCTION BOX
- IP67 PROTECTION RATING
- WORKING TEMPERATURE: -20 °C +60 °C
- 4/6 WIRES LOAD CELLS CONNECTION

DESCRIPTION		CODE
EQUALIZATION BOARD		
	■ Up to 4 load cells connection. ■ 4+1 polyamid cable glands M16x1.5 - plugs. ■ Lightning and electrical shock protection device.	CE41INOX
	■ Up to 8 load cells connection. ■ 8+1 polyamid cable glands M16x1.5 - plugs. ■ Lightning and electrical shock protection device.	CE81INOX
	■ Up to 4 load cells connection. ■ 4+1 polyamid cable glands M12x1.5 - plugs.	CE41INOXP
PARALLEL CONNECTION BOARD		
	■ Up to 4 load cells connection. ■ 4+1 polyamid cable glands M12x1.5 - plugs.	C41INOXP

JUNCTION BOXES

AISI 304 STAINLESS STEEL



TÍN THÀNH TIẾN

LAUMAS®

www.laumas.com

CERTIFICATIONS



Complies with the Eurasian Customs Union regulations

Equivalent of the CE marking for the United Kingdom



CÔNG TY TNHH CƠ KHÍ - CÂN ĐIỆN TỬ - TỰ ĐỘNG

TÍN THÀNH TIẾN®

Địa chỉ: 229A, Nguyễn Xiển, KP. Ích Thạnh, P. Trường Thạnh
TP. Thủ Đức, TP.HCM

Hot Line: 028 3746 2222

Call: 0976 879 371

Email: sale09@tttscale.com

JUNCTION BOXES

AISI 304 STAINLESS STEEL




TÍN THÀNH TIẾN

LAUMAS®


www.laumas.com

DIMENSIONS (mm)


CE41INOX

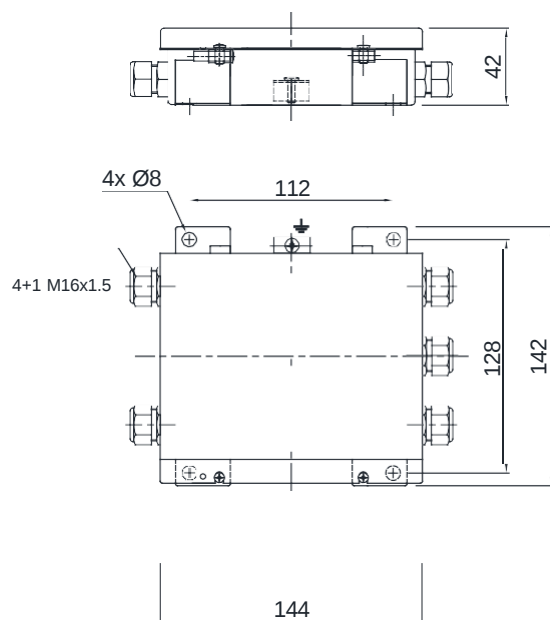

CE81INOX

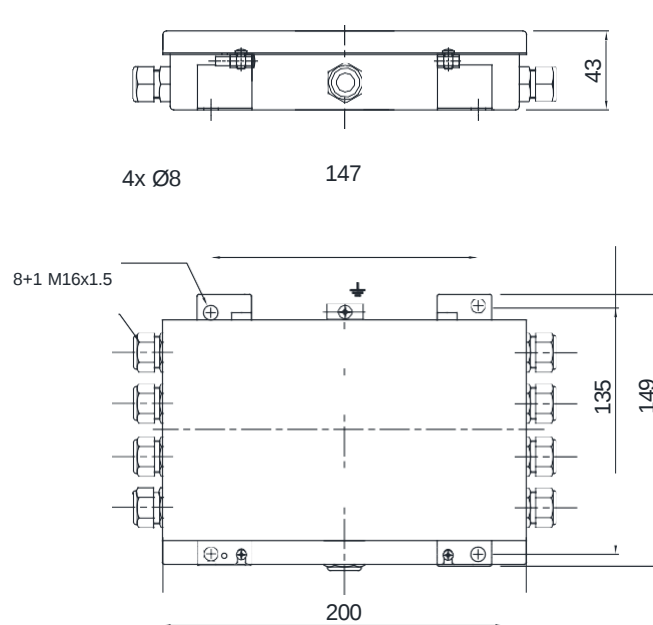

CE41INOXP - C41INOXP

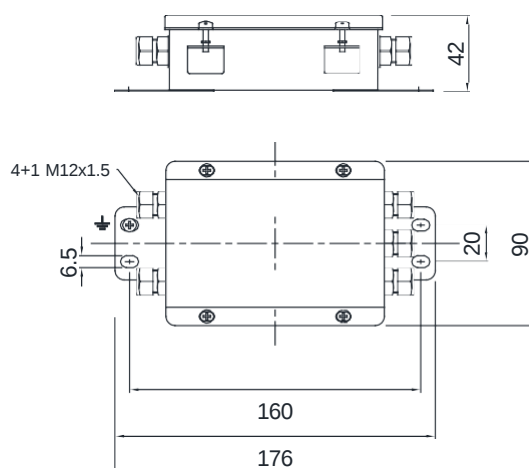

JUNCTION BOXES

AISI 304 STAINLESS STEEL




TÍN THÀNH TIẾN

LAUMAS®


www.laumas.com

ELECTRICAL CONNECTIONS


CE41INOX

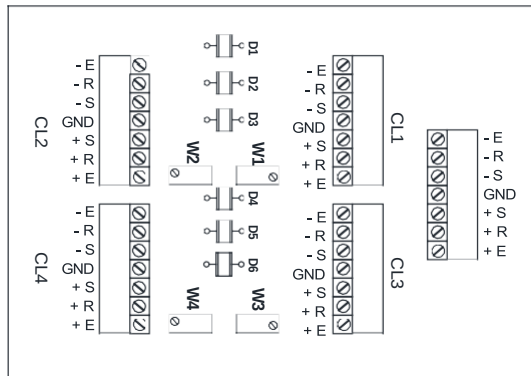


6-WIRES LOAD CELLS CONNECTION

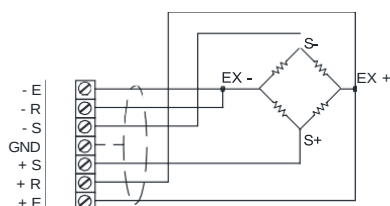


COLLEGAMENTO CELLE A 4 FILI
4-WIRES LOAD CELLS CONNECTION

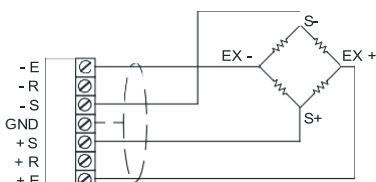


4-WIRES OUTPUT CABLE
WITH 4 WIRES LOAD CELL




6-WIRES OUTPUT CABLE
WITH 6 WIRES LOAD CELL



6-WIRES OUTPUT CABLE
WITH 4 WIRES LOAD CELL




CE81INOX

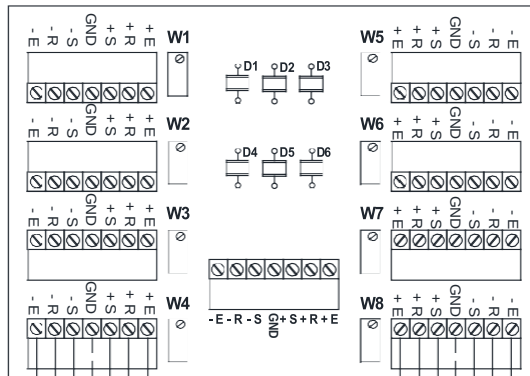

6-WIRES LOAD CELLS
CONNECTION



COLLEGAMENTO
4-WIRES LOAD CELLS
CONNECTION

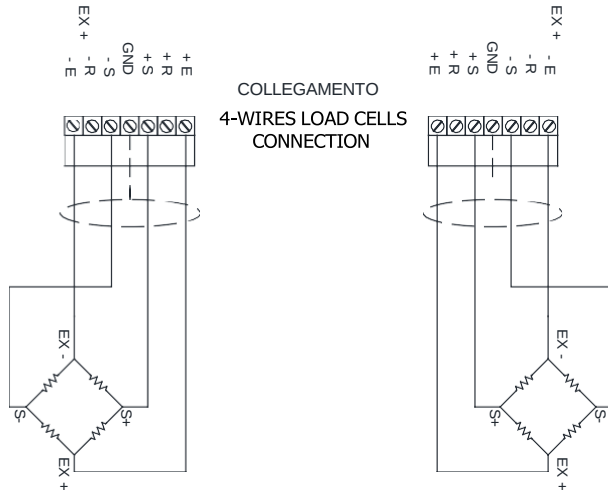

CÔNG TY TNHH CƠ KHÍ - CÂN ĐIỆN TỬ - TỰ ĐỘNG

TÍN THÀNH TIẾN®

Địa chỉ: 229A, Nguyễn Xiển, KP. Ích Thạnh, P. Trường Thạnh
TP. Thủ Đức, TP.HCM


Hot Line: 028 3746 2222

Call: 0976 879 371


Email: sale09@tttscale.com

ELECTRICAL CONNECTIONS


CE41INOXP

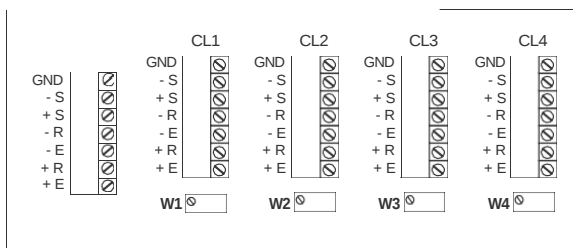


C41INOXP

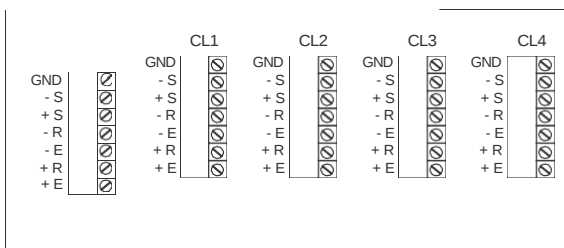


6-WIRES LOAD CELLS CONNECTION

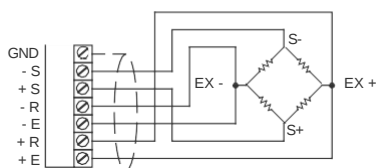


4-WIRES LOAD CELLS CONNECTION

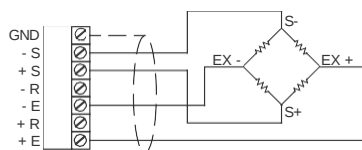


**4-WIRES OUTPUT CABLE
WITH 4 WIRES LOAD CELL**



**6-WIRES OUTPUT CABLE
WITH 6 WIRES LOAD CELL**



**6-WIRES OUTPUT CABLE
WITH 4 WIRES LOAD CELL**



EQUALIZATION PROCEDURE

WARNING!

- For load cells with 2 mV/V sensitivity the difference between the sensitivities must not be greater than 0.1 mV.
- For load cells with 3 mV/V sensitivity the difference between the sensitivities must not be greater than 0.15 mV.
- The board is equipped with a 20 Ω potentiometer for each load cell.

Example with 4 load cells and a sample weight of 978 kg:

- Turn the potentiometers'screw counterclockwise until to 0 Ω .
- Place the sample weight in correspondence with the CL1 load cell and take note of the value shown on the display; repeat the same operation for all load cells.
Example: CL1 = 1008 kg CL2 = 998 kg
CL3 = 973 kg CL4 = 985 kg
- Adjust the potentiometers related to the higher weight values (W1, W2, W4), leaving the lowest one unchanged (W3).
- Place the sample weight in correspondence with the CL1 load cell; by adjusting the potentiometer W1 change the value shown on the display from 1008 kg to 973 kg.
- Place the sample weight in correspondence with the CL2 load cell; by adjusting the potentiometer W2 change the value shown on the display from 998 kg to 973 kg.
- Place the sample weight in correspondence with the CL4 load cell; by adjusting the potentiometer W3 change the value shown on the display from 985 kg to 973 kg.
- Place the sample weight in correspondence with the CL3 load cell and take note of the value shown on the display, for example 966 kg.
- Place the sample weight in correspondence with the CL1 and adjust the potentiometer W1 until 966 kg is displayed.
- Place the sample weight in correspondence with the CL2 and adjust the potentiometer W2 until 966 kg is displayed.

10. Place the sample weight in correspondence with the CL4 and adjust the potentiometer W3 until 966 kg is displayed.
11. Place the sample weight in correspondence with the CL3 and take note of the value shown on the display, for example 962 kg.
12. Repeat the procedure several times until the display shows the same weight value for all four load cells.
13. Remove the sample weight and zero the tare, then place the sample weight in the middle and calibrate the instrument (see the instrument's user manual).

The Company reserves the right to make changes to the technical data, drawings and images without notice.